

Operating Instructions

For Model TN002Ki compact infrared thermometer


The thermometer is a non-contact infrared thermometer.

USE:

Simply aim the thermometer at the target with the probe and press the meas. Button to display the surface temperature. The distance to target diameter ratio (Distance:Spot) is 1:1 therefore the device should be positioned as close to the target as possible.

°C/ °F:

The temperature unit can be changed from °C to °F by pressing the pick hole under the back cover with a pointed object.

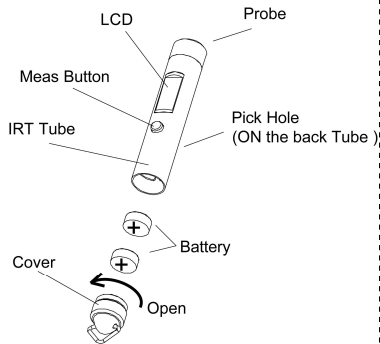

Battery Replacement:

When the above icon flash in the LCD, that indicates the battery is low and should be replaced. Confirm the unit is power OFF, loosen the cover in an anti-clockwise direction and replace the LR44 1.5v cell battery*2pcs.

** Dispose of used battery properly and keep away from children.

Measurement Range:	-33~220 °C (-27.4~428 °F)
Operating Range:	0~50 °C (32~122 °F)
Storage Range:	-20~65 °C (-4~149 °F)
Accuracy (Tamb=23±3 °C):	+/-2% of reading or 2 °C (4 °F) whichever is greater
Resolution(-9.9~199.9 °C):	0.1 °C /0.1 °F, otherwise 1 °C/1 °F
Response Time (90%):	1sec
Emissivity Range:	0.95 fixed
Auto switching-off:	15sec

Manufactured by Radiant Innovation Inc. [Http://www.ZyTemp.com](http://www.ZyTemp.com)
Add: 1F, No.3, Industrial E. 9th Rd., Science-based Industrial Park, HsinChu, Taiwan 300

Ref.No. : 032011



Operating Instructions

For Model TN002Ki compact infrared thermometer


The thermometer is a non-contact infrared thermometer.

USE:

Simply aim the thermometer at the target with the probe and press the meas. Button to display the surface temperature. The distance to target diameter ratio (Distance:Spot) is 1:1 therefore the device should be positioned as close to the target as possible.

°C/ °F:

The temperature unit can be changed from °C to °F by pressing the pick hole under the back cover with a pointed object.

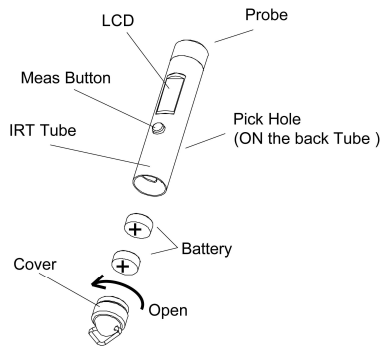

Battery Replacement:

When the above icon flash in the LCD, that indicates the battery is low and should be replaced. Confirm the unit is power OFF, loosen the cover in an anti-clockwise direction and replace the LR44 1.5v cell battery*2pcs.

** Dispose of used battery properly and keep away from children.

Measurement Range:	-33~220 °C (-27.4~428 °F)
Operating Range:	0~50 °C (32~122 °F)
Storage Range:	-20~65 °C (-4~149 °F)
Accuracy (Tamb=23±3 °C):	+/-2% of reading or 2 °C (4 °F) whichever is greater
Resolution(-9.9~199.9 °C):	0.1 °C /0.1 °F, otherwise 1 °C/1 °F
Response Time (90%):	1sec
Emissivity Range:	0.95 fixed
Auto switching-off:	15sec

Manufactured by Radiant Innovation Inc. [Http://www.ZyTemp.com](http://www.ZyTemp.com)
Add: 1F, No.3, Industrial E. 9th Rd., Science-based Industrial Park, HsinChu, Taiwan 300

Ref.No. : 032011



Operating Instructions

For Model TN002Ki compact infrared thermometer


The thermometer is a non-contact infrared thermometer.

USE:

Simply aim the thermometer at the target with the probe and press the meas. Button to display the surface temperature. The distance to target diameter ratio (Distance:Spot) is 1:1 therefore the device should be positioned as close to the target as possible.

°C/ °F:

The temperature unit can be changed from °C to °F by pressing the pick hole under the back cover with a pointed object.

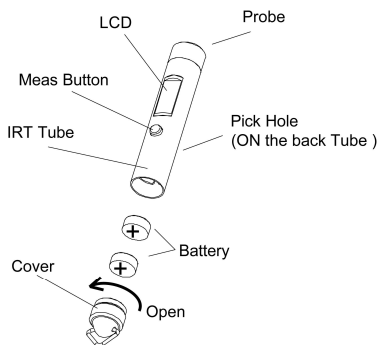

Battery Replacement:

When the above icon flash in the LCD, that indicates the battery is low and should be replaced. Confirm the unit is power OFF, loosen the cover in an anti-clockwise direction and replace the LR44 1.5v cell battery*2pcs.

** Dispose of used battery properly and keep away from children.

Measurement Range:	-33~220 °C (-27.4~428 °F)
Operating Range:	0~50 °C (32~122 °F)
Storage Range:	-20~65 °C (-4~149 °F)
Accuracy (Tamb=23±3 °C):	+/-2% of reading or 2 °C (4 °F) whichever is greater
Resolution(-9.9~199.9 °C):	0.1 °C /0.1 °F, otherwise 1 °C/1 °F
Response Time (90%):	1sec
Emissivity Range:	0.95 fixed
Auto switching-off:	15sec

Manufactured by Radiant Innovation Inc. [Http://www.ZyTemp.com](http://www.ZyTemp.com)
Add: 1F, No.3, Industrial E. 9th Rd., Science-based Industrial Park, HsinChu, Taiwan 300

Ref.No. : 032011



Operating Instructions

For Model TN002Ki compact infrared thermometer


The thermometer is a non-contact infrared thermometer.

USE:

Simply aim the thermometer at the target with the probe and press the Button to display the surface temperature. The distance to target diameter ratio (Distance:Spot) is 1:1 therefore the device should be positioned as close to the target as possible.

°C/ °F:

The temperature unit can be changed from °C to °F by pressing pick hole under the back cover with a pointed object.

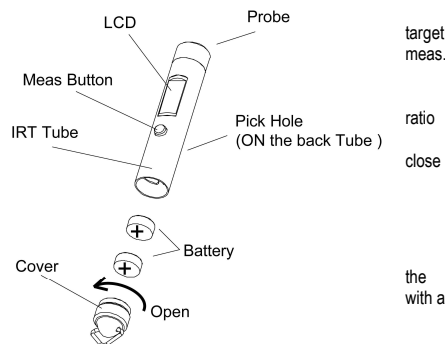

Battery Replacement:

When the above icon flash in the LCD, that indicates the battery is low and should be replaced. Confirm the unit is power OFF, loosen the cover in an anti-clockwise direction and replace the LR44 1.5v cell battery*2pcs.

** Dispose of used battery properly and keep away from children.

Measurement Range:	-33~220 °C (-27.4~428 °F)
Operating Range:	0~50 °C (32~122 °F)
Storage Range:	-20~65 °C (-4~149 °F)
Accuracy (Tamb=23±3 °C):	+/-2% of reading or 2 °C (4 °F) whichever is greater
Resolution(-9.9~199.9 °C):	0.1 °C /0.1 °F, otherwise 1 °C/1 °F
Response Time (90%):	1sec
Emissivity Range:	0.95 fixed
Auto switching-off:	15sec

Manufactured by Radiant Innovation Inc. [Http://www.ZyTemp.com](http://www.ZyTemp.com)
Add: 1F, No.3, Industrial E. 9th Rd., Science-based Industrial Park, HsinChu, Taiwan 300

Ref.No. : 032011

